

75	Journal of Optometry
76	Journal of Optometry
77	Journal of Optometry
78	Journal of Optometry
79	Journal of Optometry
80	Journal of Optometry
81	Journal of Optometry
82	Journal of Optometry
83	Journal of Optometry
84	Journal of Optometry
85	Journal of Optometry
86	Journal of Optometry
87	Journal of Optometry
88	Journal of Optometry
89	Journal of Optometry
90	Journal of Optometry
91	Journal of Optometry
92	Journal of Optometry
93	Journal of Optometry
94	Journal of Optometry
95	Journal of Optometry
96	Journal of Optometry
97	Journal of Optometry
98	Journal of Optometry
99	Journal of Optometry
100	Journal of Optometry
101	Journal of Optometry
102	Journal of Optometry
103	Journal of Optometry
104	Journal of Optometry
105	Journal of Optometry
106	Journal of Optometry
107	Journal of Optometry
108	Journal of Optometry
109	Journal of Optometry
110	Journal of Optometry
111	Journal of Optometry
112	Journal of Optometry
113	Journal of Optometry
114	Journal of Optometry
115	Journal of Optometry
116	Journal of Optometry
117	Journal of Optometry
118	Journal of Optometry
119	Journal of Optometry
120	Journal of Optometry
121	Journal of Optometry
122	Journal of Optometry
123	Journal of Optometry
124	Journal of Optometry
125	Journal of Optometry
126	Journal of Optometry
127	Journal of Optometry
128	Journal of Optometry
129	Journal of Optometry
130	Journal of Optometry
131	Journal of Optometry
132	Journal of Optometry
133	Journal of Optometry
134	Journal of Optometry
135	Journal of Optometry
136	Journal of Optometry
137	Journal of Optometry
138	Journal of Optometry
139	Journal of Optometry
140	Journal of Optometry
141	Journal of Optometry
142	Journal of Optometry
143	Journal of Optometry
144	Journal of Optometry
145	Journal of Optometry
146	Journal of Optometry

## ORIGINAL ARTICLE

# Comparison of Keeler Pulsair EasyEye tonometer and Ocular Response Analyzer for measuring intraocular pressure in healthy eyes

Carmen Lopez-De La Fuente<sup>a,\*</sup>, Ana Sanchez-Cano<sup>a</sup>, Antonio Ferreras<sup>b,c</sup>, Isabel Fuertes-Lazaro<sup>b,c</sup>

<sup>a</sup> Applied Physics Department, University of Zaragoza, Zaragoza, Spain

<sup>b</sup> Department of Ophthalmology, Miguel Servet University Hospital, Aragon Health Sciences Institute, Zaragoza, Spain

<sup>c</sup> Department of Surgery, Gynecology and Obstetrics, University of Zaragoza, Zaragoza, Spain

Received 3 February 2012; accepted 10 June 2012

Available online 19 July 2012

## KEYWORDS

Intraocular pressure;  
Noncontact  
tonometry;  
Glaucoma;  
Corneal biomechanics

## Abstract

**Purpose:** To evaluate the relationship between intraocular pressure (IOP) measurements obtained with Pulsair EasyEye (PEE) and Ocular Response Analyser (ORA) in healthy patients.

**Methods:** Sixty-five eyes from 65 patients underwent a full optometric examination, including central corneal thickness (CCT), and IOP measured with PEE and ORA. Differences between IOP measurements between both tonometers were analyzed. Pearson correlation coefficients between IOP values and ORA corneal biomechanics parameters were also obtained.

**Results:** Statistically significant differences were found between IOP of PEE (IOPk) and Goldmann-corrected IOP of ORA (IOPg;  $p=0.001$ ). IOPk and corneal resistance-corrected IOP of ORA (IOPcc) were also found to differ significantly ( $p=0.025$ ). Mean differences between IOPg-IOPk, IOPcc-IOPk and IOPg-IOPcc were  $0.71 \pm 1.66$ ,  $0.70 \pm 2.46$  and  $0.01 \pm 1.54$  mmHg (mean  $\pm$  standard deviation), respectively.

Pearson correlation coefficients indicated that IOPk, IOPg, and IOPcc were significantly correlated among them ( $p < 0.001$ ):  $r=0.816$  for IOPk-IOPg,  $r=0.826$  for IOPcc-IOPg and  $r=0.587$  IOPcc-IOPk. IOPk and IOPg were linearly associated with corneal resistance factor (CRF;  $r=0.626$  and  $r=0.619$ , respectively) and with CCT ( $r=0.531$  and  $r=0.579$ , respectively). IOPcc had a linear relationship with corneal hysteresis (CH) ( $r=-0.482$ ) and similar results were found between CRF and CH ( $r=0.841$ ), CRF and CCT ( $r=0.681$ ) or between CH and CCT ( $r=0.466$ ).

**Conclusions:** Differences between mean values of IOP measured with PEE and ORA are statistically significant, with ORA tonometer taking higher IOP values than PEE in most of the cases. IOPk, IOPcc and IOPg have, at least, moderate positive linear correlations and ORA biomechanics parameters CRF, CH and CCT have a linear positive relation between them.

© 2012 Spanish General Council of Optometry. Published by Elsevier España, S.L. All rights reserved.

\* Corresponding author at: Facultad de Ciencias, Física Aplicada, C/Pedro Cerbuna, 12, 50009 Zaragoza, Spain.

E-mail address: carmenlf@unizar.es (C. Lopez-De La Fuente).

**PALABRAS CLAVE**

Presión intraocular;  
Tonometría de no  
contacto;  
Glaucoma;  
Biomecánica corneal

## Comparación de los tonómetros Pulsair EasyEye de Keeler y el Analizador de Respuesta Ocular para la medición de la presión intraocular en ojos sanos

**Resumen**

**Objetivo:** Evaluar la relación entre las mediciones de la presión intraocular (PIO) obtenidas mediante Pulsair EasyEye (PEE) y el Analizador de Respuesta Ocular (ORA) en pacientes sanos. **Métodos:** Sesenta y cinco ojos pertenecientes a 65 pacientes recibieron un examen optométrico completo, que incluía la medición del espesor corneal central (ECC) y la PIO, con PEE y ORA. Se analizaron las diferencias entre las mediciones de PIO realizadas con ambos tonómetros. También se calcularon los coeficientes de correlación de Pearson entre los valores de PIO y los parámetros biomecánicos corneales proporcionados por el ORA.

**Resultados:** Se hallaron diferencias estadísticamente significativas entre la PIO medida con PEE (PIOk) y la PIO corregida de Goldman medida con ORA (PIOg;  $p=0,001$ ). La PIOk y la PIO corneal compensada medida con ORA (PIOcc) también fueron significativamente diferentes ( $p=0,025$ ). Las diferencias medias entre PIOg-PIOk, PIOcc-PIOk y PIOg-PIOcc fueron de  $0,71 \pm 1,66$ ,  $0,70 \pm 2,46$  y  $0,01 \pm 1,54$  mmHg (desviación media  $\pm$  estándar), respectivamente.

Los coeficientes de correlación de Pearson indicaron que los valores de PIOk, PIOg, PIOcc se hallaban significativamente correlacionados ( $p < 0,001$ ):  $r=0,816$  para PIOk-PIOg,  $r=0,826$  para PIOcc-PIOg y  $r=0,587$  PIOcc-PIOk. Los valores de PIOk y PIOg se relacionaban linealmente con el factor de resistencia corneal (FRC;  $r=0,626$  y  $r=0,619$ , respectivamente) y con el ECC ( $r=0,531$  y  $r=0,579$ , respectivamente). La PIOcc también se relacionaba linealmente con la histéresis corneal (HC;  $r=-0,482$ ), hallándose resultados similares entre la FRC y HC ( $r=0,841$ ), FRC y ECC ( $r=0,681$ ), o entre la HC y el ECC ( $r=0,466$ ).

**Conclusiones:** Las diferencias entre los valores medios de la PIO, medidas con PEE y ORA son estadísticamente significativas, obteniendo el tonómetro ORA unos valores de PIO superiores a los obtenidos por PEE en la mayoría de los casos. Los valores de PIOk, PIOcc y PIOg presentan, como mínimo, unas correlaciones lineales positivas moderadas, y los parámetros biomecánicos medidos con ORA, como FRC, HC y ECC presentan una relación positiva lineal entre ellos.

© 2012 Spanish General Council of Optometry. Publicado por Elsevier España, S.L. Todos los derechos reservados.

**Introduction**

Glaucoma is defined as an acquired optic neuropathy, which is characterized by alterations in the visual field, and some specific changes in the optic disc and retinal nerve fiber layer (RNFL).<sup>1</sup>

IOP elevation is one of the risk factors of glaucoma, and although its presence or absence does not imply disease, it can indicate that the risk of damage on the optic nerve increases with elevation of IOP.

The fact that noncontact tonometry is a convenient procedure for the patient (no need for anesthetic and the reduction of cross infection between patients) has lead to an increase in popularity of noncontact tonometers for IOP screening.<sup>2</sup> Previous articles reported very high repeatability and correlation in results between Goldmann applanation and pneumatic tonometry.<sup>3,4</sup>

The PEE (Ophthalmic Instruments Inc., UK) and the ORA (Reichert, Inc., Depew, NY) are noncontact pneumatic tonometers. The air tonometers have the same basic principal as the Goldman tonometry, but with differences in the procedure for obtaining the measurement, although it should be considered that the dependence of the corneal thickness is similar in the applanation tonometry by Goldman and the noncontact tonometry.<sup>5-7</sup>

The PEE is a portable hand-held tonometer that makes it a useful method for monitoring IOP in patients with reduced mobility, children and domiciliary visits. The PEE is one of the few tonometers capable of measuring IOP in the

supine position or in the prone position.<sup>8</sup> PEE seems to be an accurate, reliable measurement technique of IOP in the normotensive population and an alternative method in screening of IOP and when GAT is difficult to perform with certain patients.<sup>9</sup>

The ORA has been designed to compensate the effects of corneal irregularities on the measurement of the IOP using biomechanical corneal indicators.<sup>3</sup>

The ORA generates two separate IOP output parameters, corneal compensated IOP (IOPcc), which is a measurement of the IOP less affected by the corneal properties and Goldmann-correlated IOP (IOPg) which would be the traditional measurement of the IOP. The ORA provides, apart from the IOP measurements, two corneal biomechanical parameters, corneal hysteresis (CH) and corneal resistance factor (CRF). During the ORA measurement, a jet of air is projected onto the eye, which makes the shape of the cornea change, going from convex to concave. In this process, the cornea goes through a first applanation, passing through a concavity state, and achieving a second applanation state as the eye recovers its normal convex shape, once the pressure applied diminishes. The ORA software detects these two states of applanation and measures the pressure necessary to achieve them. The applanation pressure values are different, due to the viscoelastic properties of the cornea. The difference between these two pressure values is called CH and is measured in mm Hg. The CH is a measurement of corneal viscous damping, in other words, the capacity of the tissue to absorb and dissipate the energy, resulting from

the viscoelastic properties of the cornea. It is related to the state of the corneal fibers and indirectly with the CCT. The CRF measures the global resistance of the cornea which is determined by viscous resistance and its elasticity.<sup>10</sup>

There are studies that have shown that a low CH is an indicator independent of glaucomatous damage. The CH was significantly less in diseased eyes than in healthy eyes.<sup>11</sup>

Since the introduction of the ORA in clinical practice, several studies have been carried out looking for a relation between hysteresis and different pathologies apart from glaucoma and different surgical treatments. According to some authors, CH appears reduced in cases of keratoconus,<sup>12–14</sup> Fuchs' dystrophy<sup>15</sup> and even after refractive surgery and penetrating keratoplasty.<sup>12,16,17</sup>

The first objective of this study is to compare the measurements of two noncontact tonometers, PEE and ORA and to see the correlation of their measurements. The second objective is to study corneal biomechanic properties and its relationship with the IOP, starting from the values provided by the ORA (CH, CRF, CCT) in healthy population. To our knowledge, there was not any study comparing measurements between PEE and ORA.

## Methods

### Subjects

A total of 65 normal eyes of volunteers were recruited from September 2010 to November 2010. The subjects were selected from University of Zaragoza; all were students or teachers of Optics and Optometry Degree. The design of the study followed the tenets of the Declaration of Helsinki for biomedical research and the Institutional Review Board approved the study protocol. Written consent was obtained from all participants.

Exclusion criteria were previous ocular surgery, systemic diseases with ocular implications, presence of keratitis, and current use of medication that affects IOP or medications that could alter the properties of the cornea.

All patients included in this study underwent biomicroscopy of the anterior segment, IOP measurements by PEE (Keeler, Ophthalmic Instruments Inc., UK) and ORA (Reichert Inc., Depew, NY), and central corneal ultrasonic pachymetry by ORA (version 1.10 software was installed). After the procedure was explained to the subject, the readings were obtained accurately and quickly. For the assessment of IOP with PEE, three readings were taken and averaged to get the IOP reading for one eye.<sup>9</sup> A single measurement of CCT was taken for each eye with the ORA. The PEE values were taken before ORA<sup>18</sup> and at the end we obtained the CCT to avoid the effect of topical anesthesia on corneal biomechanical properties. All measurements were made at the same time of day (11 am  $\pm$  1 h) to avoid diurnal fluctuations of IOP.<sup>19</sup>

### Pneumatic tonometry (Pulsair EasyEye and Ocular Response Analyser) and central corneal thickness

Pneumatic noncontact tonometry utilizes a gentle puff of air that creates pressure on the cornea when a correct alignment with the patient's eye exists. PEE only takes measures of the IOP (IOPk) while ORA determine corneal

biomechanical properties relating the applied displacement produced in the tissue. ORA is able to measure CH that is a measurement of the ability of the cornea to both absorb and dissipate energy and the CRF that is calculated from the CH parameter and quantifies the overall corneal rigidity or stiffness.<sup>8</sup> The last parameter measured with ORA is CCT; one drop of the topical anesthetic tetracaine hydrochloride and oxybuprocaine hydrochloride (Colircusi Double anesthetic; Alcon Laboratories Inc., Fort Worth, TX) was instilled in both eyes to measure it. Data points were monitored for accuracy in ORA using the corneal waveform graph obtained with each measurement. If the waveform graph suggested an inaccurate measurement, those data points were discarded and another measurement was taken. The same experienced technician performed all explorations and other person was the responsible of recording the values.

### Statistical analyses

Statistical analyses were carried out with the Statistical Package for the Social Sciences (SPSS 17.0, SPSS Inc., Chicago, IL) and MedCal 11.0.1. (MedCal Software, Mariakerke, Belgium). Kolmogorov–Smirnov Z-test was performed to check the normal distribution of variables. As the points had Gaussian distribution, parametric tests like *t*-Student's and Pearson coefficient correlation were used. The degree of correlation was categorized, in absolute values, as low when  $r < 0.4$ , moderate when  $0.4 \leq r < 0.6$  and strong when  $0.6 \leq r$ .

The assessment of agreement between results of IOPk, IOPg and IOPcc was performed according to Bland Altman.<sup>20</sup>

Regression Graphs were performed using Excel 2003 (Microsoft® Office Excel 2003, Microsoft Corporation) and Bland–Altman plots were obtained with MedCal.

## Results

The study sample included 65 eyes from 65 healthy individuals (30% male and 70% female) with mean age  $22.6 \pm 6.7$  years, ranging from 18 to 45 years. Mean IOPk was  $14.42 \pm 2.74$  mmHg, while mean Goldmann-corrected IOP of ORA (IOPg) was  $15.13 \pm 2.71$  mmHg and corneal resistance-corrected IOP of ORA (IOPcc) was  $15.11 \pm 2.65$  mmHg. Biomechanics corneal parameters measured with ORA were  $10.91 \pm 1.39$  mmHg for CH,  $10.73 \pm 1.50$  mmHg for CRF and  $552.02 \pm 33.78$   $\mu$ m for CCT (Table 1).

### Comparison between instruments

Table 2 presents the two-tailed *t*-Student's test for the IOP measured with the Keeler tonometer and the ORA. The results (mean  $\pm$  standard deviation) indicated that there were statistically significant differences between IOPg and IOPk ( $0.71 \pm 1.66$ ;  $p = 0.001$ ) as well as between IOPcc and IOPk ( $0.70 \pm 2.46$ ;  $p = 0.025$ ). There was no significant difference between IOPg and IOPcc ( $0.01 \pm 1.54$ ;  $p = 0.952$ ).

Table 3 shows Pearson's correlation coefficients (*r*) and significance levels for two-tailed test (*p*) between the ORA measures and the Keeler tonometer values. IOPk, IOPg and IOPcc were significantly correlated between them ( $p < 0.05$ ) and these variables were found to be linearly related.

**Table 1** Descriptive statistics.

	Mean	SD ( $\pm$ )	Minimum	Maximum
Age (years)	22.6	6.7	18	45
IOPk (mmHg)	14.42	2.74	10.00	21.00
IOPg (mmHg)	15.13	2.71	9.93	20.87
IOPcc (mmHg)	15.11	2.65	9.83	22.83
CRF (mmHg)	10.73	1.50	7.63	14.97
CH (mmHg)	10.91	1.39	8.37	14.83
CCT ( $\mu$ m)	552.02	33.78	485.00	636.80

IOPk, Keeler Intraocular Pressure; IOPg, Goldmann Correlated Intraocular Pressure; IOPcc, Corneal Compensated Intraocular Pressure; SD, standard deviation; CCT, central corneal thickness; CH, corneal hysteresis; CRF, corneal resistance factor.

**Table 2** *t*-Student's test for two-tailed test.  $p \leq 0.05$  was considered statistically significant.

	Mean	SD ( $\pm$ )	<i>p</i>
IOPg vs IOPk	0.71	1.66	0.001
IOPcc vs IOPk	0.70	2.46	0.025
IOPg vs IOPcc	0.01	1.54	0.952

The degree of agreement between instruments was evaluated using the Bland-Altman method (Figs. 1–3). This analysis shows that although the limits of agreement and average difference change, the differences did not vary in direct proportion to the magnitude of the measured IOP. IOPg and IOPcc provide similar values as observed by the narrow confidence interval but IOPk shows poorer agreement with IOPcc than with IOPg like Pearson correlation coefficients do. Figs. 4–6 presents the percentage of subjects whose means differences between the IOP

measured with ORA and Keeler were within 1 mmHg, between 2.1 and 3 mmHg and over 3.1 mmHg.

### Factors affecting IOP measurements

There were statistically significant correlations between the IOP values obtained with the tonometers and the corneal biomechanical parameters (Table 3). IOPk, IOPg, IOPcc and CCT were significantly correlated between them ( $p < 0.05$ ) and these variables were also linearly related. IOPk and IOPg were linearly associated with CRF ( $r = 0.626$  and  $r = 0.619$  respectively,  $p < 0.001$ ) but not with CH ( $r = 0.232$  and  $r = 0.096$  respectively,  $p > 0.05$ ). However, the opposite occurs with IOPcc, linear relation with CH ( $r = -0.482$ ,  $p < 0.001$ ) but not with CRF ( $r = 0.069$ ,  $p > 0.05$ ). It could be also observed that all the biomechanics parameters (CRF, CH and CCT) were linearly related ( $p < 0.001$ ): CRF-CH with  $r = 0.841$ , CRF and CCT with 0.691 and CH and CCT  $r = 0.466$ .


### Discussion

Non-invasive tonometry is an objective, quick and accurate technique to measure IOP. Thus, an easy to use tonometer is necessary in optometric practice, as well as for routine checkups, glaucoma diagnosis in compromised corneas or pediatric patients. Keeler and ORA tonometers carry out this premise and they are widely incorporated in optometric protocols. These tonometers have certain advantages over the applanation tonometer, as corneal anesthesia is not required, the procedure is comfortable for the patient and there is minimal risk of corneal abrasion or cross infection between patients. It has been widely described that the non-contact tonometer ORA is considered an accurate reliable method but it cannot be used interchangeably with the GAT


**Table 3** Pearson's correlation coefficients (*r*) and significance levels for two-tailed test (*p*) between the ORA measurements and the Keeler tonometer values.  $p \leq 0.05$  was considered statistically significant.

	IOPg	IOPcc	CRF	CH	CCT
<i>IOPk</i>					
<i>r</i>	0.816	0.587	0.626	0.232	0.531
<i>p</i>	<0.001	<0.001	<0.001	0.063	<0.001
<i>IOPg</i>					
<i>r</i>	1.000	0.826	0.619	0.096	0.579
<i>p</i>		<0.001	<0.001	0.448	<0.001
<i>IOPcc</i>					
<i>r</i>		1.000	0.069	-0.482	0.247
<i>p</i>			0.583	<0.001	0.047
<i>CRF</i>					
<i>r</i>			1.000	0.841	0.681
<i>p</i>				<0.001	<0.001
<i>CH</i>					
<i>r</i>				1.000	0.466
<i>p</i>					<0.001

IOPk, Keeler Intraocular Pressure; IOPg, Goldmann Correlated Intraocular Pressure; IOPcc, Corneal Compensated Intraocular Pressure; CCT, Central corneal thickness; CH, corneal hysteresis; CRF, corneal resistance factor.

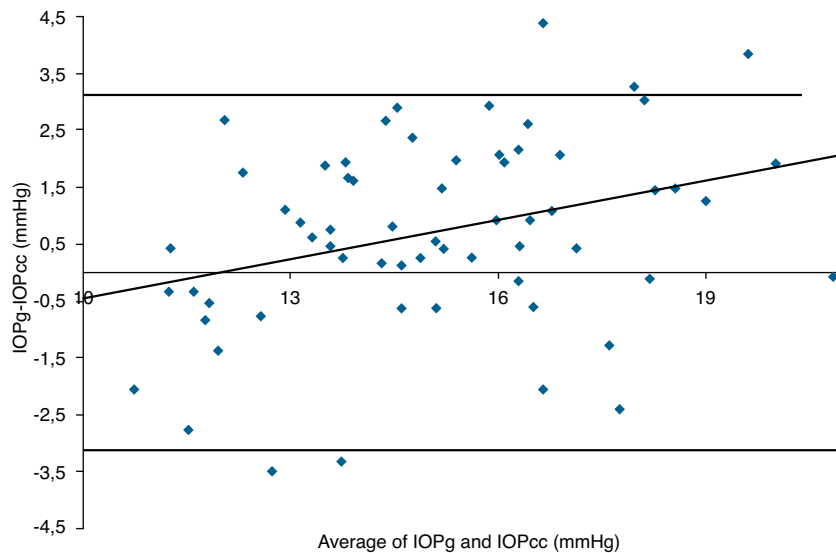

**Figure 1** Bland-Altman analysis showing distribution of intraocular pressure differences (IOPg-IOPcc) on y-axis and the average of the instruments' readings  $(IOPg + IOPcc)/2$  on the x-axis. Overall agreement is low (mean  $\Delta \pm SD$ :  $0.0 \pm 3.1$  mmHg with 95% limits of agreement between  $-3.1$  and  $+3.1$ ). Correlation  $R^2 = 0.0013$  ( $p = 0.7766$ ). Slope =  $-0.0222$  ( $p = 0.7766$ ). Intercept =  $0.3233$  ( $p = 0.7872$ ).

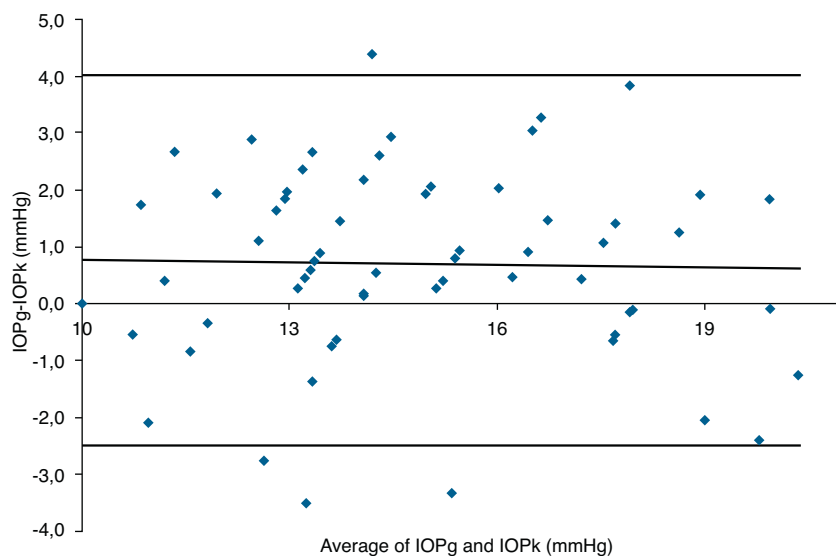

**Figure 2** Bland-Altman analysis showing distribution of intraocular pressure differences (IOPg-IOPk) on y-axis and the average of the instruments' readings  $(IOPg + IOPk)/2$  on the x-axis. Overall agreement is low (mean  $\Delta \pm SD$ :  $0.7 \pm 3.3$  mmHg with 95% limits of agreement between  $-2.5$  and  $+4.0$ ). Correlation  $R^2 = 0.0005$  ( $p = 0.8614$ ). Slope =  $-0.0141$  ( $p = 0.8614$ ). Intercept =  $0.9175$  ( $p = 0.4486$ ).


because the first overestimates IOP and differences between both sets of measurements increase with highest IOPs.<sup>21-23</sup>

IOPg and GAT present better correlation than IOPcc and GAT because viscoelastic corneal properties influence in IOPg and GAT but not in IOPcc because it is modified by the values of CH and CRF.<sup>21-23</sup>

With both tonometers, IOP average values for healthy subjects were similar to those found by other authors.<sup>9,15,24-27</sup>

Analyzing absolute values measured in the same individual we found that in the majority of the cases Keeler tonometer measured lower than the ORA did. Specifically,

IOPg was higher than IOPk in 69.23% of the cases versus 29.39% in which the opposite occurred. Average IOPcc was higher than IOPk in 66.15% of our patients, in 32.3% the contrary happened and only in 1.54% were equal. The statistical analysis of this situation revealed that significant differences were present between IOPk and IOPg and between IOPk and IOPcc. In consequence of this we can infer that both tonometers, PEE and ORA, are not clinically interchangeable. Results obtained with ORA demonstrate that between IOPg and IOPcc did not appear to exist statistically significant differences as other authors have already described.<sup>10,26,27</sup>

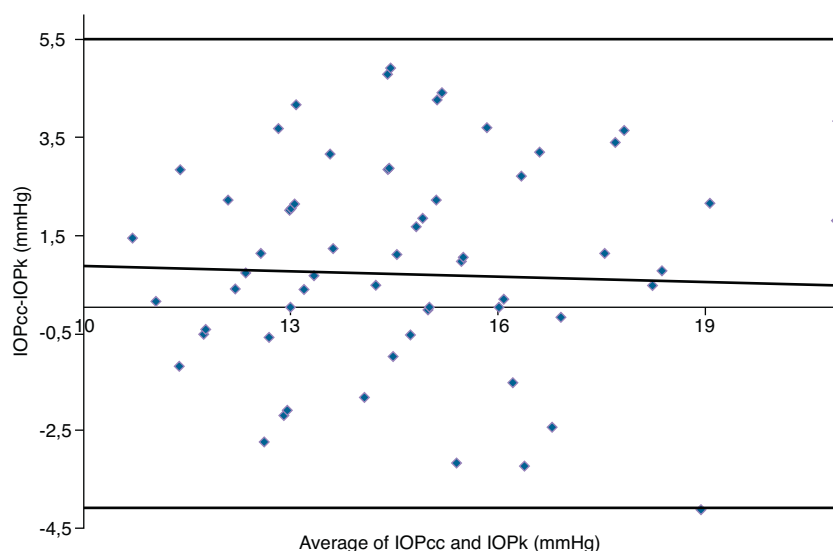


**Figure 3** Bland–Altman analysis showing distribution of intraocular pressure differences (IOPcc-IOPk) on y-axis and the average of the instruments' readings (IOPcc+IOPk)/2 on the x-axis. Overall agreement is low (mean  $\Delta \pm$  SD:  $0.7 \pm 4.8$  mmHg with 95% limits of agreement between  $-4.1$  and  $+5.5$ ). Correlation  $R^2 = 0.0017$  ( $p = 0.7473$ ). Slope =  $-0.0416$  ( $p = 0.7473$ ). Intercept =  $1.3121$  ( $p = 0.4975$ ).


Although statistical differences between means have been found, high linear correlations appeared between IOPg and IOPcc ( $r = 0.826$  and  $p < 0.001$ ) and between IOPk and IOPg ( $r = 0.816$  and  $p < 0.001$ ). Correlation between IOPk and IOPcc was moderate ( $r = 0.587$  and  $p < 0.001$ ) but this could be justified because IOPcc was corrected by CRF.

One of the most important aims of this study was to know if differences in IOP between these tonometers would be relevant in the clinical practice. According to

the Bland–Altman plots, as it has shown in previous studies,<sup>7,14,28–32,33</sup> the precision in the IOP results with ORA (IOPg and IOPcc) and PEE (IOPk) are very good in our population, with a maximum mean of  $0.7$  mmHg. In a healthy subject we have observed that average differences among IOPk, IOPcc and IOPg measurements do not vary in direct proportion to the magnitude of the measured IOP. The Bland and Altman confidence limits and the graphics of distribution of frequency (Figs. 4–6) show that for any given eye we can expect the presence of variability. A limitation of

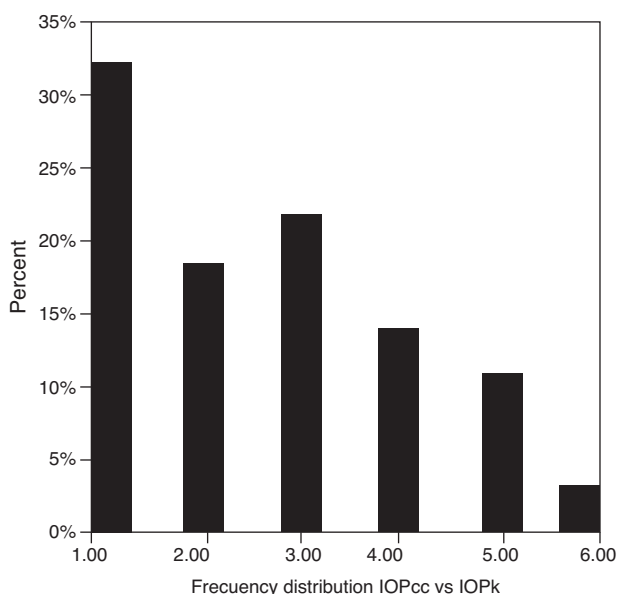


**Figure 4** Frequency distribution of absolute differences between IOPcc and IOPk (%) on y-axis and values of the difference (mmHg) on the x-axis. 0–1 mmHg (32.3%), 1.1–2 mmHg (18.5%), 2.1–3 mmHg (21.5%) and over 3.1 mmHg (27.7%).

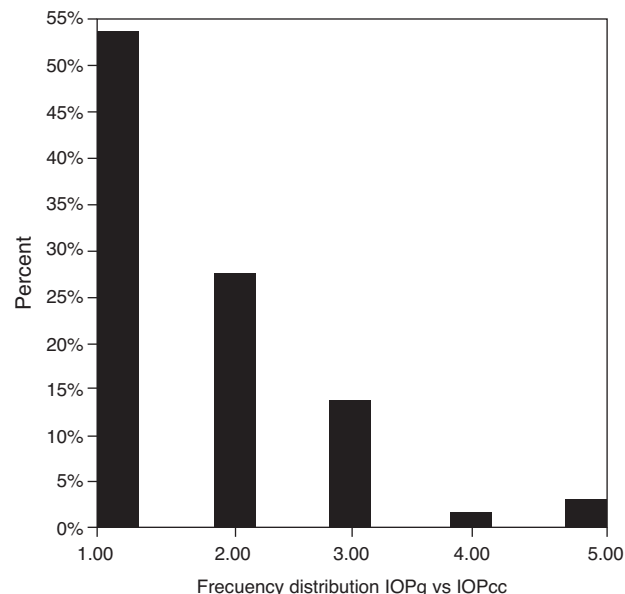

**Figure 5** Frequency distribution of absolute differences between IOPg and IOPcc (%) on y-axis and values of the difference (mmHg) on the x-axis. 0–1 mmHg (53.8%), 1.1–2 mmHg (27.7%), 2.1–3 mmHg (13.8%) and over 3.1 mmHg (4.7%).



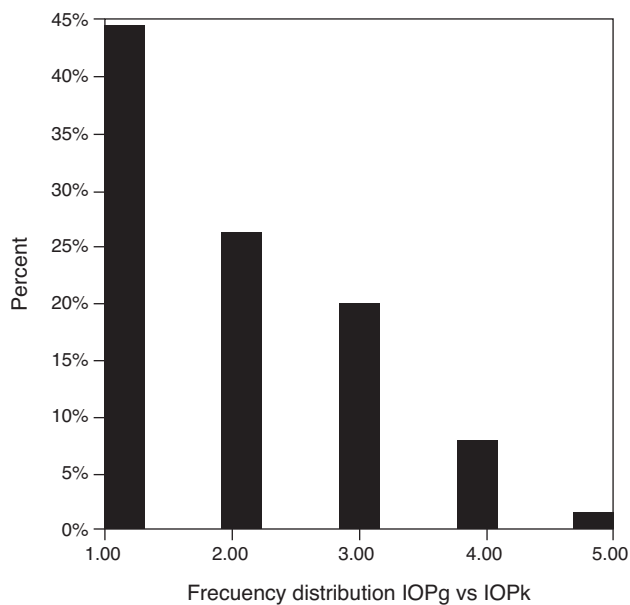

**Figure 6** Frequency distribution of absolute differences between IOPg and IOPk (%) on y-axis and values of the difference (mmHg) on the x-axis. 0–1 mmHg (44.6%), 1.1–2 mmHg (26.2%), 2.1–3 mmHg (20.0%) and over 3.1 mmHg (9.2%).

our study design is that the examiner knew the IOP previous values and for this reason could be influenced to carry out the measures in the second tonometer. In this way, more work is necessary to elucidate the possible effects of this fact in our findings.

The study of the corneal biomechanical properties was the second part of this study. Among corneal biomechanical parameters, the most previously evaluated and studied is the CH. Our mean value was 10.91 mmHg, similar to other authors except for Moreno-Montañes et al.,<sup>24</sup> who found lower results for this parameter.<sup>15,16,25–27,34–37</sup>

CH is a parameter that changes from one patient to other; our results show that in healthy eyes vary from 8.37 mmHg to 14.83 mmHg. Luce,<sup>10</sup> compared normal eyes with pathological and post-surgery eyes and their results indicated that the range of CH is higher (1.8–14.6 mmHg) in anomalous eyes than in our group. This can be explained because pathological or post-surgical eyes have lower hysteresis than healthy ones. The overlap of the ranges indicates that this parameter could not diagnose illness or surgery. In our study, like Luce,<sup>10</sup> we have observed that CH had low correlation with IOPg and IOPk and moderate with IOPcc.

Our values of CRF and CCT are similar to those found in previous studies.<sup>15–17,24–27,34–37</sup>

Correlation between CRF and CH is strong like the results previously founded by Shah et al.,<sup>16,17</sup> Montard et al.,<sup>27</sup> or other authors.<sup>10,26,32</sup>

This is due to these parameters that are obtained from the values of the flatten pressures of the tonometry. We have obtained similar results compared to these authors in the moderate correlation between CCT and CH, but a stronger correlation than Luce,<sup>10</sup> is revealed in our study. In the end, positive and high correlation between CCT and CRF is obtained in our measurements.

In conclusion, we found that PEE frequently provides lower values than the ORA does but IOPk, IOPcc and IOPg have, at least, moderate, positive linear correlations.

## References

1. Kroese M, Burton H, Vardy S, Rimmer T, McCarter D. Prevalence of primary open angle glaucoma in general ophthalmic practice in the United Kingdom. *Br J Ophthalmol*. 2002;86:978–980.
2. González-Méijome JM, Martins Jorge JM. Tonometría no invasiva. Precisión, ventajas y limitaciones (I). *Gaceta Óptica*. 2008;432:12–18.
3. Kotecha A. What biomechanical properties of the cornea are relevant for the clinician? *Surv Ophthalmol*. 2007;52(Suppl. 1):S109–S114.
4. Cho P, Lui T. Comparison of the performance of the nidek NT-2000 noncontact tonometer with the Keeler Pulsair 2000 and the goldmann applanation tonometer. *Optom Vis Sci*. 1997;74:51–58.
5. Ko YC, Liu CJ, Hsu WM. Varying effects of corneal thickness on intraocular pressure measurements with different tonometers. *Eye (Lond)*. 2005;19:327–332.
6. Recep OF, Hasiripi H, Cagil N, Sarikatipoglu H. Relation between corneal thickness and intraocular pressure measurement by noncontact and applanation tonometry. *J Cataract Refract Surg*. 2001;27:1787–1791.
7. Babalola OE, Kehinde AV, Iloegbunam AC, Akinbinu T, Moghalu C, Onuoha I. A comparison of the Goldmann applanation and non-contact (Keeler Pulsair EasyEye) tonometers and the effect of central corneal thickness in indigenous African eyes. *Ophthalmic Physiol Opt*. 2009;29:182–188.
8. Jorge J, Ramoa-Marques R, Lourenco A, et al. IOP variations in the sitting and supine positions. *J Glaucoma*. 2010;19:609–612.
9. Ogbuehi KC, Almubrad TM. Accuracy and reliability of the Keeler Pulsair EasyEye non-contact tonometer. *Optom Vis Sci*. 2008;85:61–66.
10. Luce DA. Determining in vivo biomechanical properties of the cornea with an Ocular Response Analyzer. *J Cataract Refract Surg*. 2005;31:156–162.
11. Fayol N, Abitbol O, Doan S, Duong MH, Hoang-Xuan T, Gatineau D. 167 étude de l'hystérésis cornéenne par Ocular Response Analyzer chez les sujets normaux, glaucomateux, et ayant une hypertension oculaire. *J Français d'Ophtalmol*. 2007;30(Suppl. 2):2S199.
12. Ortiz D, Piñero D, Shabayek MH, Arnalich-Montiel F, Alió JL. Corneal biomechanical properties in normal, post-laser in situ keratomileusis, and keratoconic eyes. *J Cataract Refract Surg*. 2007;33:1371–1375.
13. Albou Ganem C, Amar R. 510 éléments de corrélation entre biomécanique, topographie à élévation et pachymétrie cornéenne à partir de l'« Ocular Response Analyser® » (ORA) et de l'ORBSCAN®. *J Français d'Ophtalmol*. 2007;30(Suppl. 2):2S298.
14. Bayer A, Sahin A, Hurmeric V, Ozge G. Intraocular pressure values obtained by Ocular Response Analyzer, dynamic contour tonometry, and Goldmann tonometry in keratoconic corneas. *J Glaucoma*. 2010;19:540–545.
15. del Buey MA, Cristobal JA, Ascaso FJ, Lavilla L, Lanchares E. Biomechanical properties of the cornea in Fuchs' corneal dystrophy. *Invest Ophthalmol Vis Sci*. 2009;50:3199–3202.
16. Shah S, Laiquzzaman M, Yeung I, Pan X, Roberts C. The use of the Ocular Response Analyser to determine corneal hysteresis in eyes before and after excimer laser refractive surgery. *Contact Lens and Anterior Eye*. 2009;32:123–128.
17. Shah S, Laiquzzaman M. Comparison of corneal biomechanics in pre and post-refractive surgery and keratoconic eyes

- by Ocular Response Analyser. *Contact Lens and Anterior Eye*. 2009;32:129–132.
18. Almubrad TM, Ogbuehi KC. On repeated corneal applanation with the Goldmann and two non-contact tonometers. *Clin Exp Optom*. 2010;93:77–82.
  19. Fogagnolo P, Orzalesi N, Ferreras A, Rossetti L. The circadian curve of intraocular pressure: can we estimate its characteristics during office hours? *Invest Ophthalmol Vis Sci*. 2009;50:2209–2215.
  20. Martin Bland J, Altman D. Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet*. 1986;327:307–310.
  21. Martinez-de-la-Casa JM, Garcia-Feijoo J, Fernandez-Vidal A, Mendez-Hernandez C, Garcia-Sanchez J. Ocular Response Analyzer versus Goldmann applanation tonometry for intraocular pressure measurements. *Invest Ophthalmol Vis Sci*. 2006;47:4410–4414.
  22. Crochelet O. 407 évaluation clinique de l'Ocular Response Analyzer pour la mesure de la pression intra-oculaire. *J Français d'Ophthalmol*. 2008;31(Suppl. 1):136.
  23. Lam AK, Chen D, Tse J. The usefulness of waveform score from the Ocular Response Analyzer. *Optom Vis Sci*. 2010.
  24. Moreno-Montanes J, Maldonado MJ, Garcia N, Mendiluce L, Garcia-Gomez PJ, Segui-Gomez M. Reproducibility and clinical relevance of the Ocular Response Analyzer in nonoperated eyes: corneal biomechanical and tonometric implications. *Invest Ophthalmol Vis Sci*. 2008;49:968–974.
  25. Streho M, Dariel R, Giraud JM, et al. Evaluation of the Ocular Response Analyzer in ocular hypertension, glaucoma, and normal populations. prospective study on 329 eyes. *J Fr Ophthalmol*. 2008;31:953–960.
  26. Ehongo A, de Maertelaer V, Cullus P, Pourjavan S. Corrélation entre hystérèse cornéenne, facteur de résistance cornéen et amplitude de pulsation oculaire chez les sujets sains. *J Français d'Ophthalmol*. 2008;31:999–1005.
  27. Montard R, Kopito R, Touzeau O, et al. Ocular Response Analyzer: Étude de fiabilité et de corrélation sur des yeux normaux. *J Français d'Ophthalmol*. 2007;30:978–984.
  28. Parker VA, Herrtage J, Sarkies NJ. Clinical comparison of the Keeler Pulsair 3000 with Goldmann applanation tonometry. *Br J Ophthalmol*. 2001;85:1303–1304.
  29. Carbonaro F, Andrew T, Mackey DA, Spector TD, Hammond CJ. Comparison of three methods of intraocular pressure measurement and their relation to central corneal thickness. *Eye (Lond)*. 2010;24:1165–1170.
  30. Ehrlich JR, Haseltine S, Shimmyo M, Radcliffe NM. Evaluation of agreement between intraocular pressure measurements using Goldmann applanation tonometry and Goldmann correlated intraocular pressure by Reichert's Ocular Response Analyser. *Eye (Lond)*. 2010;24:1555–1560.
  31. Renier C, Zeyen T, Fieuws S, Vandenbroeck S, Stalmans I. Comparison of Ocular Response Analyzer, dynamic contour tonometer and Goldmann applanation tonometer. *Int Ophthalmol*. 2010.
  32. Medeiros FA, Weinreb RN. Evaluation of the influence of corneal biomechanical properties on intraocular pressure measurements using the Ocular Response Analyzer. *J Glaucoma*. 2006;15:364–370.
  33. Jorge J, Gonzalez-Mejome JM, Queiros A, Fernandes P, Diaz-Rey JA. A comparison of the NCT Reichert R7 with Goldmann applanation tonometry and the Reichert Ocular Response Analyzer. *Ophthalmic Physiol Opt*. 2011;31:174–179.
  34. Shah S, Laiquzzaman M, Cunliffe I, Mantry S. The use of the Reichert Ocular Response Analyser to establish the relationship between ocular hysteresis, corneal resistance factor and central corneal thickness in normal eyes. *Contact Lens Anterior Eye*. 2006;29:257–262.
  35. Wells AP, Garway-Heath DF, Poostchi A, Wong T, Chan KC, Sachdev N. Corneal hysteresis but not corneal thickness correlates with optic nerve surface compliance in glaucoma patients. *Invest Ophthalmol Vis Sci*. 2008;49:3262–3268.
  36. Fontes BM, Ambrósio Junior R, Jardim D, Velarde GC, Nosé W. Ability of corneal biomechanical metrics and anterior segment data in the differentiation of keratoconus and healthy corneas. *Arq Bras Oftalmol*. 2010;73:333–337.
  37. Kopito R, Gaujoux T, Montard R, et al. Reproducibility of viscoelastic property and intraocular pressure measurements obtained with the ocular response analyzer. *Acta Ophthalmol*. 2011;89:e225–e230.